



# JD EVOLUTION plus

Insertie simplă, stabilitate naturală



conexiune hexagonală




Made in Italy

## INSERȚIE SIMPLĂ, STABILITATE NATURALĂ


### caracteristici și avantaje

- Conexiune hexagonală internă cu ghidaj de introducere
- Guler coronal anatomic
- Corp interior expansiv conic
- Capacitate de auto-tăiere în ambele direcții
- Lamele de tăiere apicale
- Conexiunea este recunoscută universal de toate bibliotecile digitale principale
- Reduce concentrarea stresului pe osul crestei și maximizează volumul osului în jurul gâtului implantului pentru țesuturi dure și moi stabile
- Permite obținerea unei stabilități primare ridicate

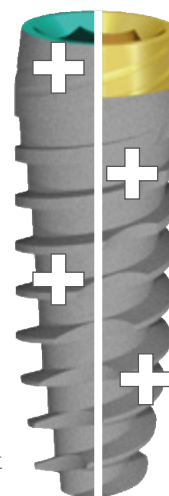

Tratament complet de suprafață SLA

Gulerul implantului anodizat de H 1,5 mm și tratamentul de suprafață SLA pe corp

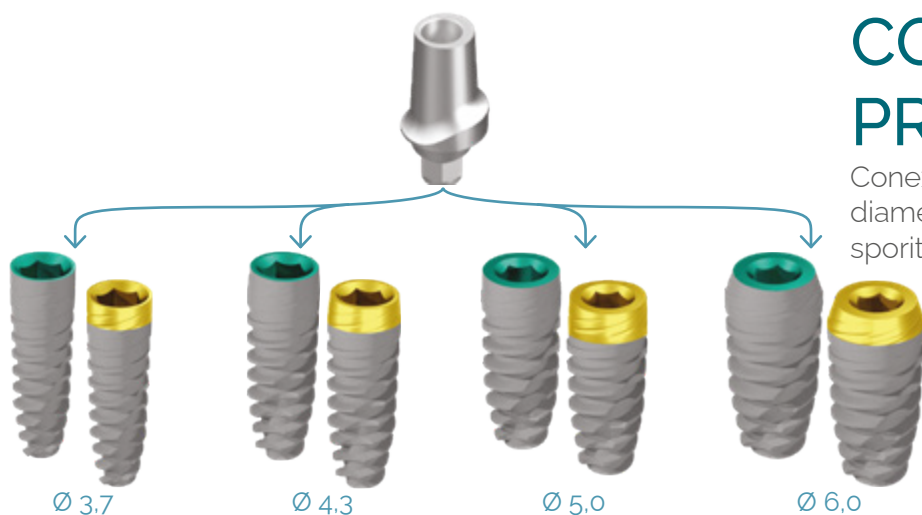



## CONEXIUNE PROTETICĂ SIMPLĂ

Conexiune protetică simplă pentru toate diametrele. Inventar redus și flexibilitate sporită în lucrul zilnic.

## CARACTERISTICELE PRODUSULUI

Implanturile dentare JDEvolution Plus sunt disponibile în diametrele și lungimile indicate în tabelul următor:

DIAMETRU IMPLANT	DIAMETRU TIP	INTERFAȚA BONTULUI	DIAMETR PLATFORMĂ	LUNGIME						
				6	8	10	11,5	13	15	18
Ø 3.7	2.4	3.4	3.7		8	10	11,5	13	15	18
Ø 4.0	2.4	3.4	3.8	6	8	10	11,5	13	15	18
Ø 4.3	2.8	3.4	4.0	6	8	10	11,5	13	15	18
Ø 5.0	3.2	3.4	4.8	6	8	10	11,5	13	15	18
Ø 6.0	4.0	3.4	5.0	6	8	10	11,5	13	15	

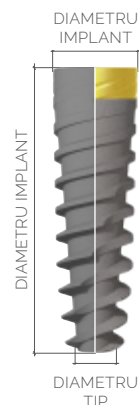

Notă: Toate dimensiunile sunt exprimate în mm.

# CATALOG DE PRODUSE

## Implanturi:

### Ø 3,7

EV37080:	JDEvolution Plus Ø 3.7 L 8
EV37100:	JDEvolution Plus Ø 3.7 L 10
EV37115:	JDEvolution Plus Ø 3.7 L 11.5
EV37130:	JDEvolution Plus Ø 3.7 L 13
EV37150:	JDEvolution Plus Ø 3.7 L 15
EV37180:	JDEvolution Plus Ø 3.7 L 18

### Ø 4,3

EV43060:	JDEvolution Plus Ø 4.3 L 6
EV43080:	JDEvolution Plus Ø 4.3 L 8
EV43100:	JDEvolution Plus Ø 4.3 L 10
EV43115:	JDEvolution Plus Ø 4.3 L 11.5
EV43130:	JDEvolution Plus Ø 4.3 L 13
EV43150:	JDEvolution Plus Ø 4.3 L 15
EV43180:	JDEvolution Plus Ø 4.3 L 18

### Ø 5,0

EV50060:	JDEvolution Plus Ø 5.0 L 6
EV50080:	JDEvolution Plus Ø 5.0 L 8
EV50100:	JDEvolution Plus Ø 5.0 L 10
EV50115:	JDEvolution Plus Ø 5.0 L 11.5
EV50130:	JDEvolution Plus Ø 5.0 L 13
EV50150:	JDEvolution Plus Ø 5.0 L 15
EV50180:	JDEvolution Plus Ø 5.0 L 18

### Ø 6,0

EV60060:	JDEvolution Plus Ø 6.0 L 6
EV60080:	JDEvolution Plus Ø 6.0 L 8
EV60100:	JDEvolution Plus Ø 6.0 L 10
EV60115:	JDEvolution Plus Ø 6.0 L 11.5
EV60130:	JDEvolution Plus Ø 6.0 L 13
EV60150:	JDEvolution Plus Ø 6.0 L 15

## Implan cu guler anodizat

### Ø 3,7

EVA37080:	JDEvolution Plus Anodized Collar Ø 3.7 L 8
EVA37100:	JDEvolution Plus Anodized Collar Ø 3.7 L 10
EVA37115:	JDEvolution Plus Anodized Collar Ø 3.7 L 11.5
EVA37130:	JDEvolution Plus Anodized Collar Ø 3.7 L 13
EVA37150:	JDEvolution Plus Anodized Collar Ø 3.7 L 15
EVA37180:	JDEvolution Plus Anodized Collar Ø 3.7 L 18

### Ø 4,3







EVA43060:	JDEvolution Plus Anodized Collar Ø 4.3 L 6
EVA43080:	JDEvolution Plus Anodized Collar Ø 4.3 L 8
EVA43100:	JDEvolution Plus Anodized Collar Ø 4.3 L 10
EVA43115:	JDEvolution Plus Anodized Collar Ø 4.3 L 11.5
EVA43130:	JDEvolution Plus Anodized Collar Ø 4.3 L 13
EVA43150:	JDEvolution Plus Anodized Collar Ø 4.3 L 15
EVA43180:	JDEvolution Plus Anodized Collar Ø 4.3 L 18

### Ø 5,0

EVA50060:	JDEvolution Plus Anodized Collar Ø 5.0 L 6
EVA50080:	JDEvolution Plus Anodized Collar Ø 5.0 L 8
EVA50100:	JDEvolution Plus Anodized Collar Ø 5.0 L 10
EVA50115:	JDEvolution Plus Anodized Collar Ø 5.0 L 11.5
EVA50130:	JDEvolution Plus Anodized Collar Ø 5.0 L 13
EVA50150:	JDEvolution Plus Anodized Collar Ø 5.0 L 15
EVA50180:	JDEvolution Plus Anodized Collar Ø 5.0 L 18

### Ø 6,0

EVA60060:	JDEvolution Plus Anodized Collar Ø 6.0 L 6
EVA60080:	JDEvolution Plus Anodized Collar Ø 6.0 L 8
EVA60100:	JDEvolution Plus Anodized Collar Ø 6.0 L 10
EVA60115:	JDEvolution Plus Anodized Collar Ø 6.0 L 11.5
EVA60130:	JDEvolution Plus Anodized Collar Ø 6.0 L 13
EVA60150:	JDEvolution Plus Anodized Collar Ø 6.0 L 15

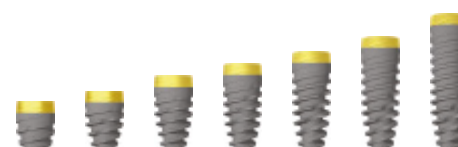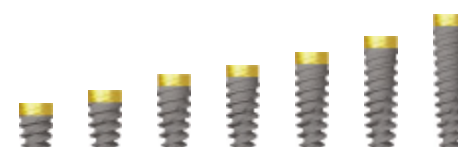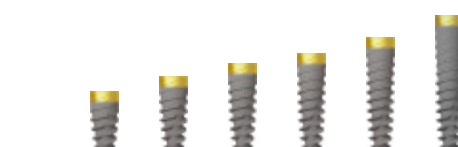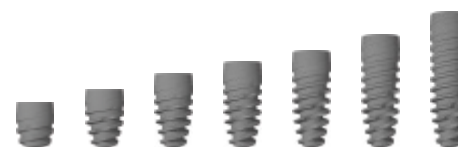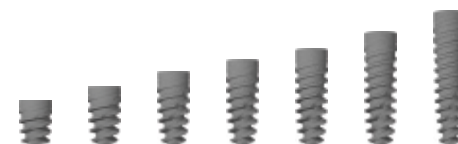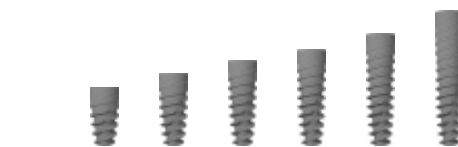

## Implanturi Ø 4,0:

EVT40060:	JDEvolution Plus Ø 4.0 L 6
EVT40080:	JDEvolution Plus Ø 4.0 L 8
EVT40100:	JDEvolution Plus Ø 4.0 L 10
EVT40115:	JDEvolution Plus Ø 4.0 L 11.5
EVT40130:	JDEvolution Plus Ø 4.0 L 13
EVT40150:	JDEvolution Plus Ø 4.0 L 15
EVT40180:	JDEvolution Plus Ø 4.0 L 18



## Șurub de acoperire:

EVCS:	Cover Screw JDEvolution Plus
EVCS6:	Cover Screw Ø 6.0 JDEvolution Plus



## Bont de vindecare:


EVHA43:	Healing Abutment Ø 4.0 H 3.0 JDEvolution Plus
EVHA45:	Healing Abutment Ø 4.0 H 5.0 JDEvolution Plus
EVHA47:	Healing Abutment Ø 4.0 H 7.0 JDEvolution Plus
EVHA53:	Healing Abutment Ø 5.0 H 3.0 JDEvolution Plus
EVHA55:	Healing Abutment Ø 5.0 H 5.0 JDEvolution Plus
EVHA57:	Healing Abutment Ø 5.0 H 7.0 JDEvolution Plus
EVHA59:	Healing Abutment Ø 5.0 H 9.0 JDEvolution Plus
EVHA63:	Healing Abutment Ø 6.0 H 3.0 JDEvolution Plus
EVHA65:	Healing Abutment Ø 6.0 H 5.0 JDEvolution Plus
EVHA67:	Healing Abutment Ø 6.0 H 7.0 JDEvolution Plus
EVHA753:	Healing Abutment Ø 7.5 H 3.0 JDEvolution Plus
EVHA755:	Healing Abutment Ø 7.5 H 5.0 JDEvolution Plus
EVHA54TS:	Healing Abutment Tissue Ø 5.0 H 4.0 JDEvolution Plus
EVHA56TS:	Healing Abutment Tissue Ø 5.0 H 6.0 JDEvolution Plus



## Copiator de amprentă:

### Tip deschis

EVICOT4C:	Impression Coping Open Tray Ø 4.0 JDEvolution Plus
EVICOT5C:	Impression Coping Open Tray Ø 5.0 JDEvolution Plus
EVICOT6C:	Impression Coping Open Tray Ø 6.0 JDEvolution Plus
EVICOTNEC:	Impression Coping Open Tray Non Engaging JDEvolution Plus
EVICOTS:	Impression Coping Open Tray Screw JDEvolution Plus
EVICOT5TSC:	Impression Coping Tissue Open Tray Ø 5.0 JDEvolution Plus

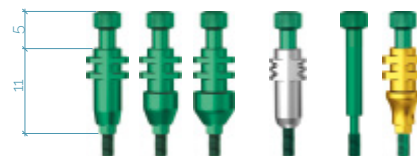

### Tip închis

EVICCT4C:	Impression Coping Closed Tray Ø 4.0 JDEvolution Plus
EVICCT5C:	Impression Coping Closed Tray Ø 5.0 JDEvolution Plus
EVICCT6C:	Impression Coping Closed Tray Ø 6.0 JDEvolution Plus
EVICCTS:	Impression Coping Closed Tray Screw JDEvolution Plus
EVICCT1C:	Impression Coping Closed Tray Direct Press Fit JDEvolution Plus



## Bont temporar:

EVTAEAC:	Temporary Abutment Engaging JDEvolution Plus
EVTAEPC:	Temporary Abutment Engaging Peek JDEvolution Plus
EVTANEC:	Temporary Abutment Non Engaging JDEvolution Plus
EVTAE TSC:	Temporary Abutment Tissue Engaging JDEvolution Plus
EVTANETSC:	Temporary Abutment Tissue Non Engaging JDEvolution Plus



Torsiunea recomandată 30 Ncm

## Bont drept:

EVNSA4510C:	Straight Abutment Ø 4.5 H 1.5 JDEvolution Plus
EVNSA4520C:	Straight Abutment Ø 4.5 H 2.0 JDEvolution Plus
EVNSA4540C:	Straight Abutment Ø 4.5 H 4.0 JDEvolution Plus
EVNSA5020C:	Straight Abutment Ø 5.0 H 2.0 JDEvolution Plus
EVNSA5040C:	Straight Abutment Ø 5.0 H 4.0 JDEvolution Plus
EVNSA6020C:	Straight Abutment Ø 6.0 H 2.0 JDEvolution Plus
EVNSA6040C:	Straight Abutment Ø 6.0 H 4.0 JDEvolution Plus
EVNSA5020TSC:	Straight Abutment Tissue Ø 5.0 H 2.0 JDEvolution Plus
EVNSA5040TSC:	Straight Abutment Tissue Ø 5.0 H 4.0 JDEvolution Plus



Torsiunea recomandată 30 Ncm

Torsiunea recomandată 30 Ncm



## Bont GP:

EV15GPAEC:	GP Abutment 15° JDEvolution Plus
EV25GPAEC:	GP Abutment 25° JDEvolution Plus

Torque recommended 30 Ncm




EVGPA4oEC:	GP Abutment Engaging Ø 4.0 JDEvolution Plus
EVGPA4oNEC:	GP Abutment Non Engaging Ø 4.0 JDEvolution Plus
EVGPAEC:	GP Abutment Engaging Ø 5.0 JDEvolution Plus
EVGPA5oNEC:	GP Abutment Non Engaging Ø 5.0 JDEvolution Plus
EVGPAEPC:	GP Abutment Engaging Peek Ø 5.0 JDEvolution Plus
EVGPA6oEC:	GP Abutment Engaging Ø 6.0 JDEvolution Plus



Torsiunea recomandată 30 Ncm

## Bont angulat anatomic:

EVEA15:	Anatomic Abutment H 1.5 JDEvolution Plus
EVEA30:	Anatomic Abutment H 3.0 JDEvolution Plus
EV15A15:	15° Angulated Anatomic Abutment Ø 5.0 H 1.5 JDEvolution Plus
EV15A15N:	15° Angulated Anatomic Abutment Ø 4.5 H 1.5 JDEvolution Plus
EV15A30:	15° Angulated Anatomic Abutment Ø 5.0 H 3.0 JDEvolution Plus
EV15A30N:	15° Angulated Anatomic Abutment Ø 4.5 H 3.0 JDEvolution Plus
EV25A15:	25° Angulated Anatomic Abutment Ø 5.0 H 1.5 JDEvolution Plus
EV25A30:	25° Angulated Anatomic Abutment Ø 5.0 H 3.0 JDEvolution Plus

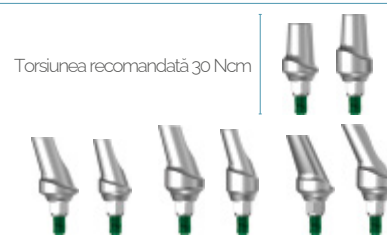

Torsiunea recomandată 30 Ncm

Torsiunea recomandată 30 Ncm

## Bont rapid:

EVRA15C:	Rapid Abutment H 1.5 JDEvolution Plus
EVRA30C:	Rapid Abutment H 3.0 JDEvolution Plus
EVRA15D:	Rapid Abutment w/o Healing Cap and Coping H 1.5 JDEvolution Plus
EVRA30D:	Rapid Abutment w/o Healing Cap and Coping H 3.0 JDEvolution Plus
EVRAHC	Rapid Abutment Healing Cap
EVRAIC	Rapid Abutment Impression Coping
EVRAAR	Rapid Abutment Replica




Torsiunea recomandată 30 Ncm

Torsiunea recomandată 30 Ncm

## Bont pentru modelare cu ceară:


EVWAEC:	Wax-Up Abutment Engaging JDEvolution Plus
EVWANEC:	Wax-Up Abutment Non Engaging JDEvolution Plus

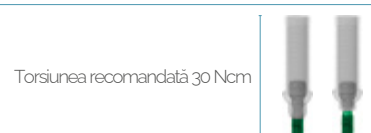

Torsiunea recomandată 30 Ncm

## Bont din cobalt-crom:

EVCCEC:	Chrome-Cobalt Abutment Engaging JDEvolution Plus
EVCCNEC:	Chrome-Cobalt Abutment Non Engaging JDEvolution Plus
EVCAACCNEC:	Cobalt-Chrome Conical Abutment Non Engaging JDEvolution Plus

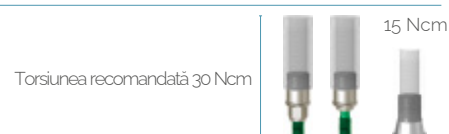


Torsiunea recomandată 30 Ncm

15 Ncm

## Bont din aur:

EVGAEC:	Gold Abutment Engaging JDEvolution Plus
EVGANEC:	Gold Abutment Non Engaging JDEvolution Plus

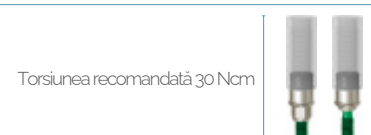

Torsiunea recomandată 30 Ncm

## Bont conic multiunit (MUA)

EVNCA10C:	Conical Abutment Straight H 1.0 JDEvolution Plus
EVNCA15C:	Conical Abutment Straight H 1.5 JDEvolution Plus
EVNCA20C:	Conical Abutment Straight H 2.0 JDEvolution Plus
EVNCA30C:	Conical Abutment Straight H 3.0 JDEvolution Plus
EVNCA40C:	Conical Abutment Straight H 4.0 JDEvolution Plus
EVNCA70C:	Conical Abutment Straight H 7.0 JDEvolution Plus
EVNCA90C:	Conical Abutment Straight H 9.0 JDEvolution Plus
EVNCA15TSC:	Conical Abutment Tissue Straight H 1.5 JDEvolution Plus
EVNCA30TSC:	Conical Abutment Tissue Straight H 3.0 JDEvolution Plus
EVNCA40TSC:	Conical Abutment Tissue Straight H 4.0 JDEvolution Plus
EVNCA50TSC:	Conical Abutment Tissue Straight H 5.0 JDEvolution Plus
EVCA1725C:	Conical Abutment Angulated 17° H 2.5 JDEvolution Plus
EVCA1735C:	Conical Abutment Angulated 17° H 3.5 JDEvolution Plus
EVCA3025C:	Conical Abutment Angulated 30° H 2.5 JDEvolution Plus
EVCA3035C:	Conical Abutment Angulated 30° H 3.5 JDEvolution Plus
EVCA1725TSC:	Conical Abutment Tissue Angulated 17° H 2.5 JDEvolution Plus
EVCA1735TSC:	Conical Abutment Tissue Angulated 17° H 3.5 JDEvolution Plus
EVA275C:	Conical Abutment Tissue Angulated 17° H 5.0 JDEvolution Plus
EVCA3025TSC:	Conical Abutment Tissue Angulated 30° H 2.5 JDEvolution Plus
EVCA3035TSC:	Conical Abutment Tissue Angulated 30° H 3.5 JDEvolution Plus
EVCA3050TSC:	Conical Abutment Tissue Angulated 30° H 5.0 JDEvolution Plus



Torsiunea recomandată 30 Ncm



Torsiunea recomandată 30 Ncm



Torsiunea recomandată 30 Ncm



Torsiunea recomandată 30 Ncm

EVA137C:	Conical Abutment Straight Engaging H 1.5 JDEvolution Plus
EVA138C:	Conical Abutment Straight Engaging H 3.0 JDEvolution Plus
EVS105:	Screw for Conical Abutment Straight Engaging H 1.5 JDEvolution Plus
EVS106:	Screw for Conical Abutment Straight Engaging H 3.0 JDEvolution Plus
EVCASA:	Screw for Angulated Conical Abutment JDEvolution Plus
EVCAPS:	Prosthetic Screw Conical Abutment JDEvolution Plus
EVCAPSL:	Prosthetic Screw Conical Abutment Long JDEvolution Plus
EVCAPSA	Prosthetic Screw Angulated for Conical Abutment JDEvolution
EVCAICOTEC:	Conical Abutment Impression Coping Engaging Open Tray JDEvolution Plus
EVCAICOTC:	Conical Abutment Impression Coping Open Tray JDEvolution Plus
EVCAICOTLC:	Conical Abutment Impression Coping Open Tray Long JDEvolution Plus
EVCAICOT2:	Screw for Conical Abutment Impression Coping Open Tray JDEvolution Plus
EVCAICOT4:	Screw for Conical Abutment Impression Coping Open Tray Long JDEvolution Plus
EVCAICTC	Conical Abutment Impression Coping Closed Tray
EVCAHC:	Healing Cap for Conical Abutment JDEvolution Plus
EVCAHCL:	Conical Abutment Healing Cap H 6.0 JDEvolution Plus
EVCAHCg:	Conical Abutment Healing Cap H 9.0 JDEvolution Plus
EVCAHCB:	Conical Abutment Healing Cap Peek JDEvolution Plus
EVCAGPAEC:	GP Abutment Engaging for Conical Abutment JDEvolution Plus
EVCAGPANEC:	GP Abutment Non Engaging for Conical Abutment JDEvolution Plus
EVCATANEWSC:	Temporary Abutment Non Engaging Conical Abutment Smooth for Welding JDEvolution Plus
EVCATANEC:	Temporary Abutment Non Engaging Conical Abutment JDEvolution Plus
EVCATANEWC:	Temporary Abutment Non Engaging Conical Abutment for Welding JDEvolution Plus
EVCAWANEC:	Wax-Up Abutment Non Engaging for Conical Abutment JDEvolution Plus
EVCAAR	Conical Abutment Replica



Torsiunea recomandată 30 Ncm




Torsiunea recomandată 30 Ncm



Torsiunea recomandată 30 Ncm



Torsiunea recomandată 15 Ncm



Torsiunea recomandată 15 Ncm

## Şurub protetic:

EVS:	Prosthetic Screw JDEvolution Plus
EVSA:	Prosthetic Screw Angulated JDEvolution Plus

Torsiunea recomandată 30 Ncm



## Interfețe:

EVINTEC:	Interface Engaging JDEvolution Plus
EVINTNEC:	Interface Non Engaging JDEvolution Plus
70287C:	Interface Non Engaging for Conical Abutment JDEvolution Plus

Torsiunea recomandată 30 Ncm




15 Ncm

## Bont AS:

EVASCEC:	AS Abutment Engaging JDEvolution Plus
EVASCNEC:	AS Abutment Non Engaging JDEvolution Plus

Torsiunea recomandată 30 Ncm



## TiBase, JDScaBody și Implant Replica CAD CAM:

EVSBCEC:	ScanBody Engaging JDEvolution Plus
EVCASBCEC:	ScanBody Conical Abutment JDEvolution Plus
EVCASBCEEC:	ScanBody Engaging Conical Abutment JDEvolution Plus
EVCASBCEESC:	On Top ScanBody Conical Abutment JDEvolution Plus
EVHSB53:	On Top ScanBody Engaging Ø 5.0 H 3.0 JDEvolution Plus
EVHSB55:	On Top ScanBody Engaging Ø 5.0 H 5.0 JDEvolution Plus
EVHSB57:	On Top ScanBody Engaging Ø 5.0 H 7.0 JDEvolution Plus
EVSCPC:	ScanPost JDEvolution Plus



EVTIBC:	TiBase Engaging Ø4.25 H 0.5 C 4.7 JDEvolution Plus
EVTIBNEC:	TiBase Non Engaging Ø4.25 H 0.5 C 4.7 JDEvolution Plus
EVTIB15C:	TiBase Engaging Ø4.25 H 1.5 C 4.7 JDEvolution Plus
EVTIB15NEC:	TiBase Non Engaging Ø4.25 H 1.5 C 4.7 JDEvolution Plus
EVTIB30C:	TiBase Engaging Ø4.25 H 3.0 C 4.7 JDEvolution Plus
EVTIB30NEC:	TiBase Non Engaging Ø4.25 H 3.0 C 4.7 JDEvolution Plus






Torsiunea recomandată 30 Ncm




EVTIBNC:	TiBase Long Engaging Ø4.4 H 0.5 C 7.7 JDEvolution Plus
EVTIBNENC:	TiBase Long Non Engaging Ø4.4 H 0.5 C 7.7 JDEvolution Plus
EVTIB15NC:	TiBase Long Engaging Ø4.4 H 1.5 C 7.7 JDEvolution Plus
EVTIB15NENC:	TiBase Long Non Engaging Ø4.4 H 1.5 C 7.7 JDEvolution Plus
EVTIB30NC:	TiBase Long Engaging Ø4.4 H 3.0 C 7.7 JDEvolution Plus
EVTIB30NENC:	TiBase Long Non Engaging Ø4.4 H 3.0 C 7.7 JDEvolution Plus



Torsiunea recomandată 30 Ncm

EVA150C:	TiBase Long Engaging Ø4.4 H 0.5 C 7.7 for Angulated Channel JDEvolution Plus	
EVA151C:	TiBase New Non Engaging Ø4.4 H 0.5 C 7.7 for Angulated Channel JDEvolution Plus	
EVA152C:	TiBase Long Engaging Ø4.4 H 1.5 C 7.7 for Angulated Channel JDEvolution Plus	
EVA153C:	TiBase New Non Engaging Ø4.4 H 1.5 C 7.7 for Angulated Channel JDEvolution Plus	
EVA154C:	TiBase Long Engaging Ø4.4 H 3.0 C 7.7 for Angulated Channel JDEvolution Plus	
EVA155C:	TiBase New Non Engaging Ø4.4 H 3.0 C 7.7 for Angulated Channel JDEvolution Plus	
EVA133C:	Tibase Interface Engaging H 6.0 for Angulated Channel JDEvolution Plus*	
EVA134C:	Tibase Interface Non Engaging H 6.0 for Angulated Channel JDEvolution Plus*	
EVA135C:	Tibase Interface Engaging H 10.0 for Angulated Channel JDEvolution Plus*	
EVA136C:	Tibase Interface Non Engaging H 10.0 for Angulated Channel JDEvolution Plus*	

Pentru produsele indicate, șurubul protetic EVS trebuie folosit pentru canalele drepte, iar șurubul protetic EVSA trebuie folosit pentru canalele unghiulare. Șuruburile protetice nu sunt incluse.

EVCAITEC	Interface CAD CAM Engaging for Conical Abutment JDEvolution Plus (H 7.5)	
EVA139C:	TiBase Engaging for Conical Abutment JDEvolution Plus (H 5.0)	
EVCAITC:	Interface CAD CAM Non Engaging for Conical Abutment JDEvolution Plus (H 7.3)	
EVCATIBC:	TiBase for Conical Abutment JDEvolution Plus (H 5.0)	
EVA138N:	Implant Replica CAD CAM New JDEvolution Plus	
EVCAARCN	Conical Abutment Replica CAD CAM New	
EVPMNC:	Pre-milled Abutment Blank JDEvolution Plus	




Torsiunea recomandată 15 Ncm

Torsiunea recomandată 15 Ncm

Torsiunea recomandată 30 Ncm

Notă: Vă rugăm să contactați [info@jdentalcare.com](mailto:info@jdentalcare.com) pentru biblioteca digitală pentru software-urile Exocad, 3Shape și Dental Wings.


### Bont conometric:

EVCP05C:	Conometric Abutment Straight H 0.5 JDEvolution Plus	
EVCP10C:	Conometric Abutment Straight H 1.0 JDEvolution Plus	
EVCP20C:	Conometric Abutment Straight H 2.0 JDEvolution Plus	
EVCP30C:	Conometric Abutment Straight H 3.0 JDEvolution Plus	
EVCP40C:	Conometric Abutment Straight H 4.0 JDEvolution Plus	
EV7CP20C:	7.5° Angulated Conometric Abutment H 2.0 JDEvolution Plus	
EV15CP20C:	15° Angulated Conometric Abutment H 2.0 JDEvolution Plus	
EV22CP20C:	22.5° Angulated Conometric Abutment H 2.0 JDEvolution Plus	
EVA300C:	30° Angulated Conometric Abutment H 2.0 JDEvolution Plus	
EVCPS:	Screw for Conometric Abutment JDEvolution Plus	
EVA130C:	Cap With Pin for Intraoral Welding	
EVA131C:	Cap for Partial or Full-Arch Fixed Prosthesis	
EVA132C:	Anti-Rotation Cap for Single Element	
EVCPIC	Conometric Abutment Impression Coping PEEK	
EVCPAN	Conometric Abutment Replica	

Torsiunea recomandată 30 Ncm


Torsiunea recomandată 30 Ncm

### Bont sferic cu bilă cu bilă:

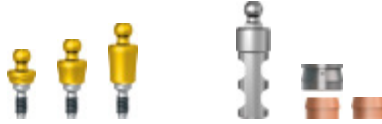EVBA15:	Ball Abutment H 1.5 JDEvolution Plus	
EVBA30:	Ball Abutment H 3.0 JDEvolution Plus	
EVBA50:	Ball Abutment H 5.0 JDEvolution Plus	
EVBAA	Ball Abutment Replica	
EVBAHC	Ball Abutment Elastic Retention Cap w/ Container	
EVBAN	Ball Abutment Retention Cap	


Torsiunea recomandată 30 Ncm

### Bont EMI:

EVEMI15:	Emi Abutment H 1.5 JDEvolution Plus	
EVEMI30:	Emi Abutment H 3.0 JDEvolution Plus	
EVEMI50:	Emi Abutment H 5.0 JDEvolution Plus	
EVEMISCK	Smart cap attachment Emi Abutment	
EVEMIHC	Emi Abutment Elastic Retention Cap w/ Container	
EVEMIN	Emi Abutment Elastic Retention Cap (1.2 kg)	
EVEMIH	Emi Abutment Container	
EVEMIIIC	Emi Abutment Plastic Impression Coping	
EVEMIIICS	Emi Abutment Steel Impression Coping	
EVEMINT	Emi Abutment White Retention Cap (1.8 kg)	
EVEMINY	Emi Abutment Yellow Retention Cap (0.6 kg)	
EVEMINP	Emi Abutment Purple Retention Cap (2.5 kg)	
EVEMINB	Emi Abutment Retention Cap for Laboratory	
EVEMIEIT	Extractor-insertion Tool For Caps	
EVEMIA	Emi Abutment Replica	

Torsiunea recomandată 30 Ncm

### Replică implant:

EVAN:	Implant Replica JDEvolution Plus	
-------	----------------------------------	---


## Moară os colector:

JDBMNNC:	Bone Mill Ø 5.0 and Guide JDEvolution Plus
JDBM6NC:	Bone Mill Ø 6.0 and Guide JDEvolution Plus
JDBMGNN:	Bone Mill Guide JDEvolution Plus



## Cheițe și dispozitive pentru impanturi și proteze:

EVID:	Implant Driver JDEvolution Plus
EVIDL:	Implant Driver Long JDEvolution Plus
JDID127	Implant Depth Aligner JDEvolution Plus
EVSDPF15:	Prosthetic Driver for JDTorque L 15 JDEvolution Plus
EVSDPF20:	Prosthetic Driver for JDTorque L 20 JDEvolution Plus
EVSDPF25:	Prosthetic Driver for JDTorque L 25 JDEvolution Plus
EVSDPF35:	Prosthetic Driver for JDTorque L 35 JDEvolution Plus
EVSDPF60:	Prosthetic Driver for JDTorque L 60 JDEvolution Plus
EVSDCAF	Conical Abutment Driver for JDTorque
EVSDP20:	Prosthetic Driver L 20 JDEvolution Plus
EVSDP25:	Prosthetic Driver L 25 JDEvolution Plus
EVSDP30:	Prosthetic Driver L 30 JDEvolution Plus
JDPD105	Prosthetic Driver JDEvolution Plus for Surgical Driver
EVSDCA	Conical Abutment Drive
EVSDPF25A	Angulated Screw Driver for JDTorque L 25
EVSDPF30A	Angulated Screw Driver for JDTorque L 30
EVSUD	Surgical Driver JDEvolution
JDG	JDGuide
EVGMC	Implant Mounter for JDEvolution
EVGMLC	Implant Mounter Long JDEvolution
JDID102	ZAPA Tool

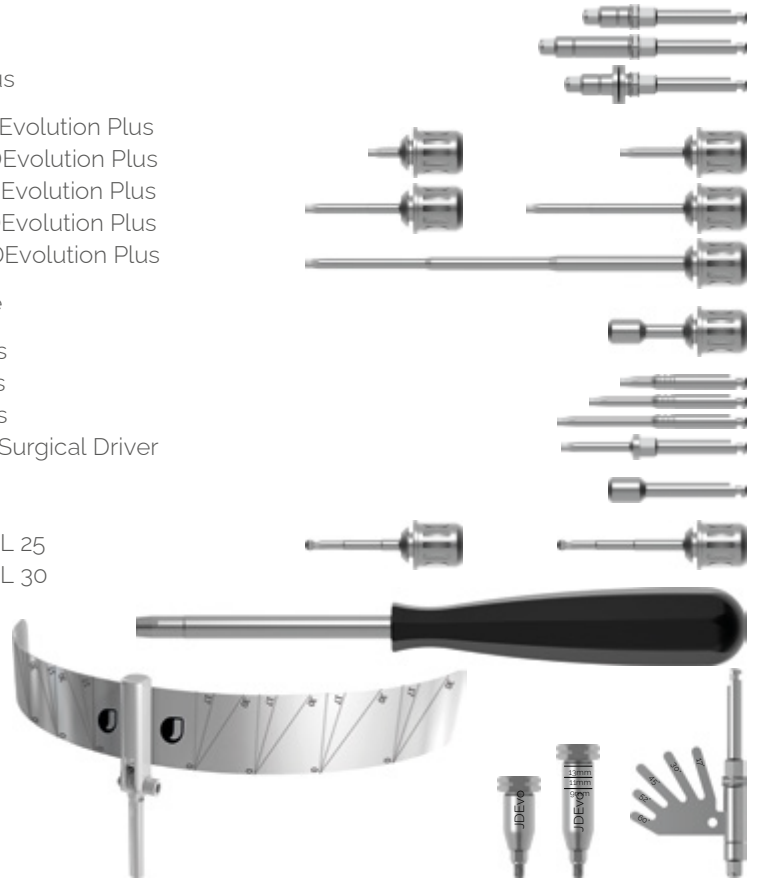

## Indicații de direcție:

JDDI	Direction Indicator
JDDIS	Direction Indicator Short
JDDI17	Direction Indicator 17°
JDDI30	Direction Indicator 30°
JDDI45	Direction Indicator 45°





# PROTOCOALE DE FORAJ

Se recomandă respectarea indicațiilor secvenței de foraj pentru a asigura stabilitatea primară optimă a implanturilor.

## Pregătirea sitului în maxilar

DIAMETRU IMPLANTULUI	OS VINDECAT		OS POST EXTRACTIV	
	OS MOALE	OS SEMIDENS	OS MOALE	OS SEMIDENS
Ø 3.7	2,0 2,4 2,8 up to the laser mark L6mm	2,0 2,4 2,8 3,2 up to the laser mark L6mm	2,0 2,4 2,8 at the entrance	2,0 2,4 2,8 at the entrance
Ø 4.3	2,0 2,4 2,8 3,2 at the entrance	2,0 2,4 2,8 3,2 up to the laser mark L6-8mm 3,6 at the entrance	2,0 2,4 2,8 3,2 at the entrance	2,0 2,4 2,8 3,2 at the entrance
Ø 5.0	2,0 2,4 2,8 3,2 3,6 up to the 1	2,0 2,4 2,8 3,2 3,6 up to the 1 4,0 at the entrance	2,0 2,4 2,8 3,2 3,6 at the entrance up to the 1	2,0 2,4 2,8 3,2 3,6 at the entrance up to the 1
Ø 6.0	2,0 2,4 2,8 3,2 3,6	2,0 2,4 2,8 3,2 3,6 4,0 4,4 up to the 1	2,0 2,4 2,8 3,2 3,6 4,0	2,0 2,4 2,8 3,2 3,6 4,0



până la prima etichetă laser L6mm



short  
Ø 4,3  
L 6


Începeți osteotomia cu burghiul standard cu spirală Ø 2,0 mm și Ø 2,4 mm  
Finalizați cu burghiul Ø 4 mm L 6 mm, codul JDDICS4 scurt Ø 5,0 L6

short  
Ø 5,0  
L 6

Începeți osteotomia cu burghiul standard cu spirală Ø 2,0 mm și Ø 2,4 mm  
Finalizați cu burghiul Ø 4 mm L 6 mm, codul JDDICS4D

## Pregătirea sitului în maxilar

DIAMETRU IMPLANTULUI	OS VINDECAT		OS POST EXTRACTIV	
	OS MOALE	OS SEMIDENS	OS MOALE	OS SEMIDENS
Ø 3.7	2,0 2,4 2,8 3,2 up to the 2 3,6 up to the 1	2,0 2,4 2,8 3,2 3,6 up to the 1	2,0 2,4 2,8 3,2 at the entrance	2,0 2,4 2,8 3,2 at the entrance
Ø 4.3	2,0 2,4 2,8 3,2 3,6 up to the 2 4,0 up to the 2	2,0 2,4 2,8 3,2 3,6 4,0 up to the 2 4,4 up to the 1	2,0 2,4 2,8 3,2 3,6 at the entrance	2,0 2,4 2,8 3,2 3,6 at the entrance
Ø 5.0	2,0 2,4 2,8 3,2 3,6 4,0 4,4 up to the 2 4,8 at the entrance	2,0 2,4 2,8 3,2 3,6 4,0 4,4 4,8 at the entrance	2,0 2,4 2,8 3,2 3,6 4,0 at the entrance	2,0 2,4 2,8 3,2 3,6 4,0 at the entrance
Ø 6.0	2,0 2,4 2,8 3,2 3,6 4,0 4,4 up to the 2 4,8 up to the 2	2,0 2,4 2,8 3,2 3,6 4,0 4,4 4,8 up to the 2	2,0 2,4 2,8 3,2 3,6 4,0 4,4	2,0 2,4 2,8 3,2 3,6 4,0 4,4



până la prima etichetă laser L6mm




short  
Ø 4,3  
L 6

Începeți osteotomia cu burghiul standard cu spirală Ø 2,0 mm și Ø 2,4 mm  
Finalizați cu burghiul Ø 4 mm L 6 mm, codul JDDICS4 scurt Ø 5,0 L6

short  
Ø 5,0  
L 6

Începeți osteotomia cu burghiul standard cu spirală Ø 2,0 mm și Ø 2,4 mm  
Finalizați cu burghiul Ø 4 mm L 6 mm, codul JDDICS4D

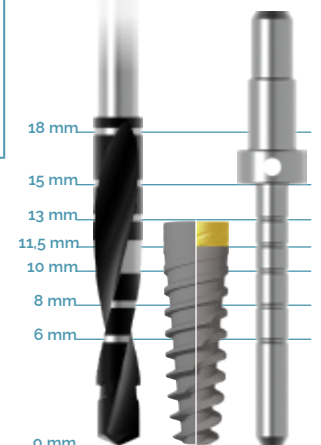

# DRILLING PROTOCOLS

It is recommended to adhere to the indications of the following drilling sequence to ensure optimal primary stability

## Pregătirea site-ului în maxilar



DIAMETRU IMPLANTULUI	OS VINDECAT		OS POST EXTRACTIV		Implant scurt L6mm DEvolution Plus introdus în maxilar.
	OS MOALE	OS SEMIDENS	OS MOALE	OS SEMIDENS	
Ø 4,0	2.0 2.4 2.8	2.0 2.4 2.8 3.2 up to the 2	2.0 2.4 2.8 up to the 2	2.0 2.4 2.8	short Ø 4,0 L 6 Începeți osteotomia cu burghiul standard cu spirală Ø 2.0 mm și Ø 2.4 mm Finalizați cu burghiul Ø 4 mm L 6 mm, codul JDDICS4 scurt Ø 5,0 L6

## Pregătirea site-ului în mandibulă



DIAMETRU IMPLANTULUI	OS VINDECAT		OS POST EXTRACTIV		Implant scurt L6mm DEvolution Plus introdus în maxilar.
	OS MOALE	OS SEMIDENS	OS MOALE	OS SEMIDENS	
Ø 4,0	2.0 2.4 2.8 3.2 up to the 2 3.6 up to the 2	2.0 2.4 2.8 3.2 3.6 4.0 up to the 1	2.0 2.4 2.8 3.2 up to the 2 3.6 up to the 1	2.0 2.4 2.8 3.2 3.6 up to the 1	short Ø 4,0 L 6 Începeți osteotomia cu burghiul standard cu spirală Ø 2.0 mm și Ø 2.4 mm Finalizați cu burghiul Ø 4 mm L 6 mm, codul JDDICS4D



**JDENTALCARE**

[www.jdentalcare.com](http://www.jdentalcare.com)



**REPREZENTANT AUTORIZAT JDENTALCARE ROMANIA**

**S.C TOPDENT TECHNIC SRL / CUI : 43646472**

**BUCURESTI , STR.BARBU VACARESCU 162**

**EMAIL : [CONTACT@ALLONX.RO](mailto:CONTACT@ALLONX.RO)**

**CONTACT : +4074492166**

**WEB : [WWW.JDENTALCARE.RO](http://WWW.JDENTALCARE.RO)**

**E-SHOP : [WWW.ALLONX.RO](http://WWW.ALLONX.RO)**